



## HEIGHT CALIBRATION OF SCANNING PROBE MICROSCOPE ACTUATORS Osamah M. El Rifai et al. Application No. 10/722,806


1/6




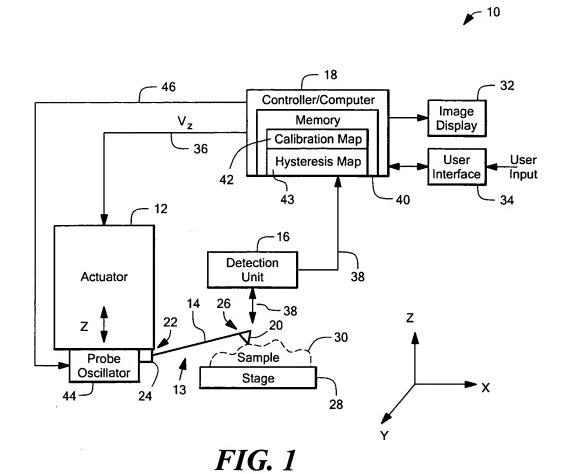


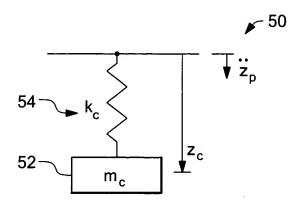

**FIG. 2** 

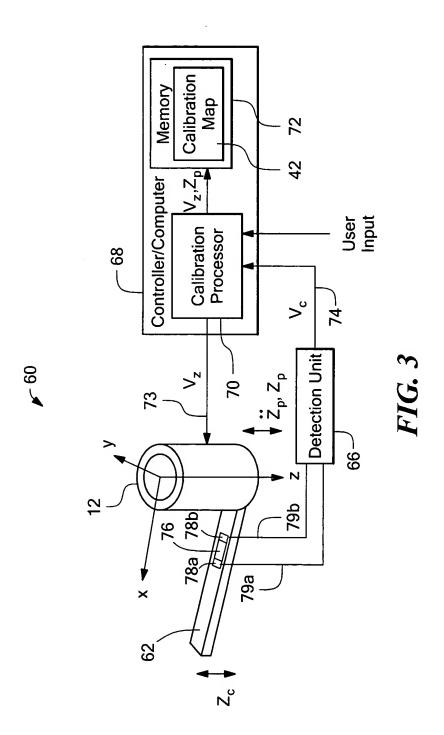

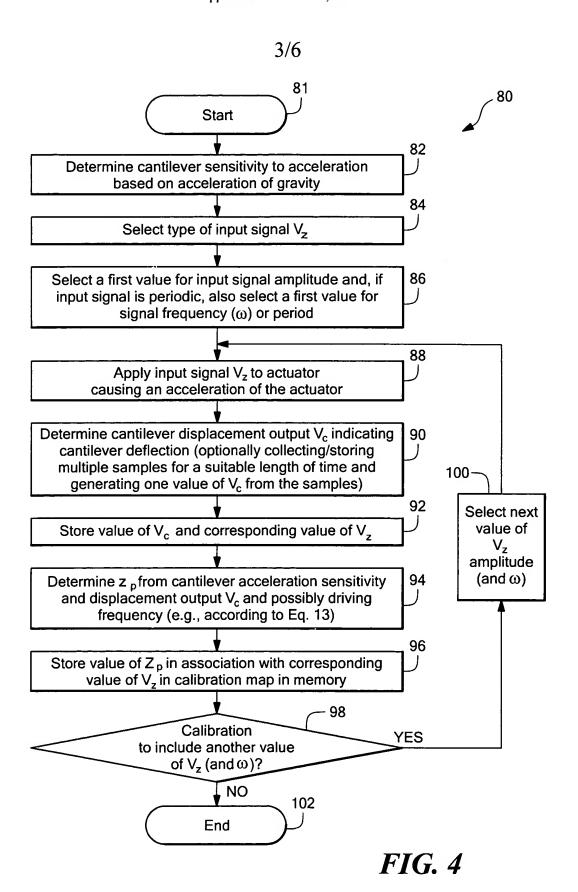

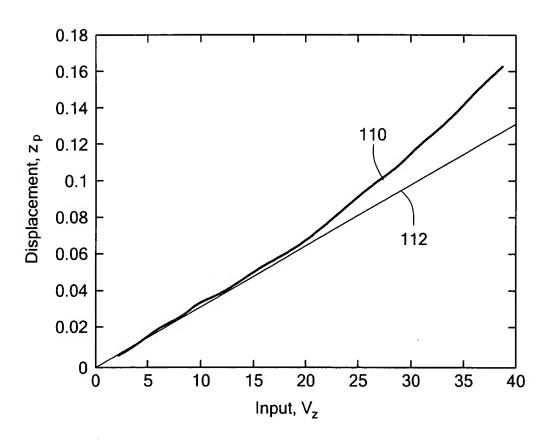

*FIG.* 5

